Manual Supplement

Manual Title:	1760 Reference	Supplement Issue:	**1**
Print Date:	July 2006	Issue Date:	2/14
Revision/Date:	2, 7/10	Page Count:	2

This supplement contains information necessary to ensure the accuracy of the above manual. This manual is distributed as an electronic manual on the following CD-ROM:

CD Title:	1760
CD Rev. & Date:	5, 7/10
CD PN:	2583518

© 2014 Fluke Corporation. All rights reserved..


FLUKE®

Change #1

On page 1-2, add the following to the **Symbols** table:

KC	Conforms to relevant South Korean EMC Standards.

On page 5-7, replace the figure with:

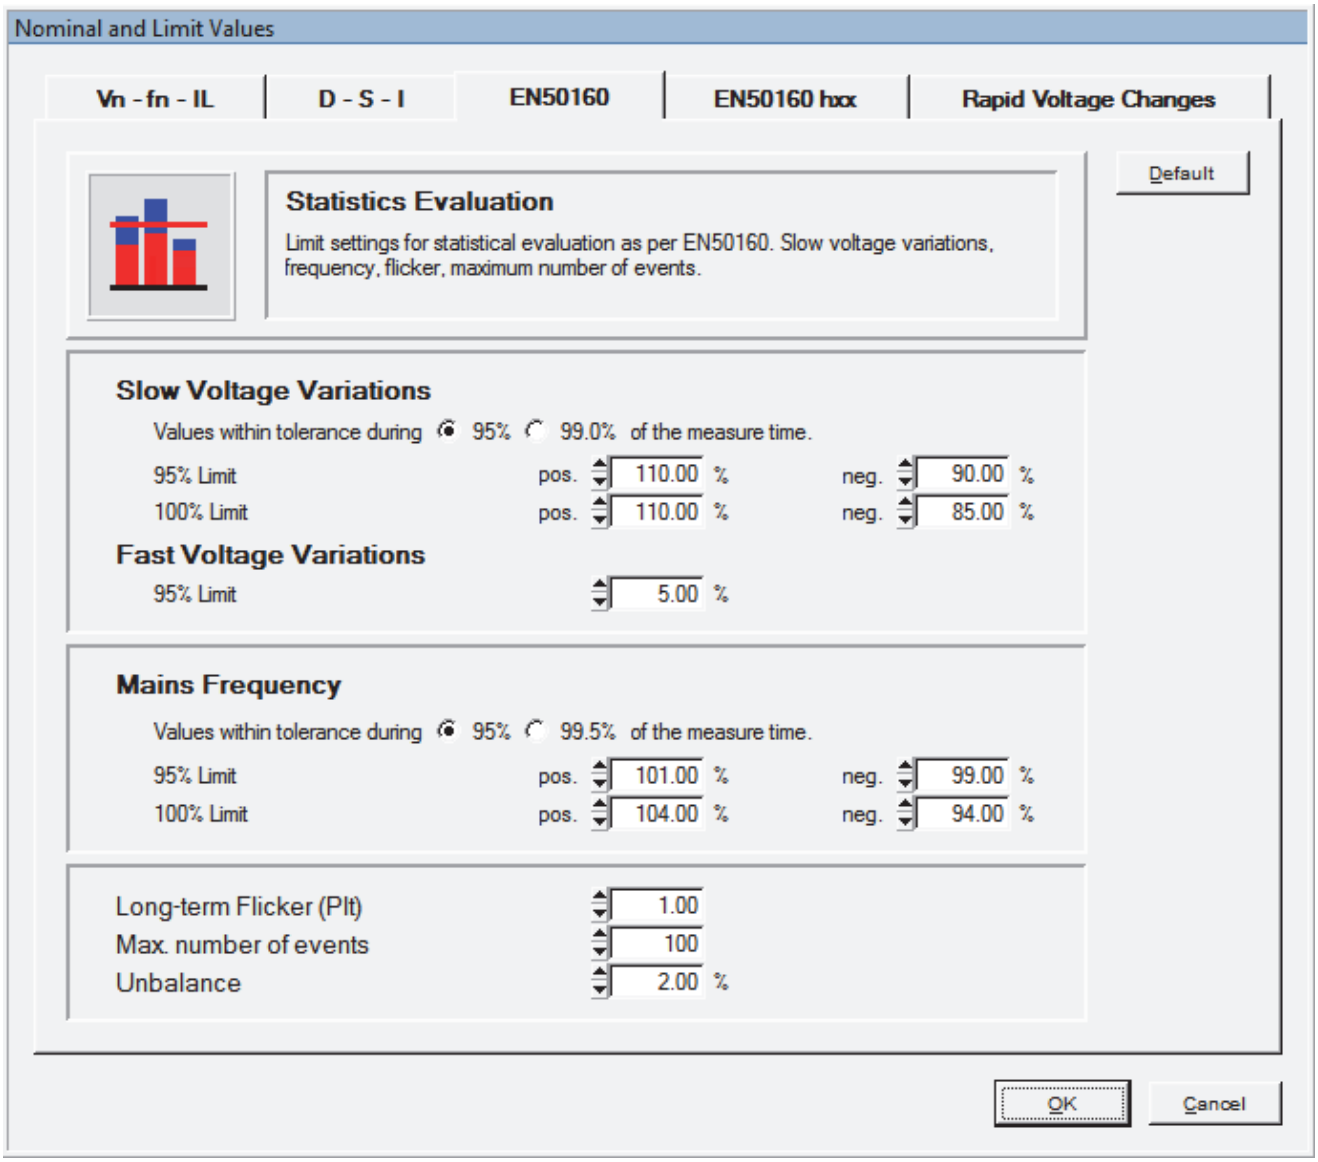

On page 6-23, add the following under the Note:

See below for a Dis/Dip table showing the distribution statistics of voltage dips depending on the length of the dip event according to EN50160:

EN50160 - Event Statistics

Voltage Swells 3-ph:

Swell Voltage [%Vnom]	Duration [ms]		
	½cyc <= t <= 500	500 < t <= 5000	5000 < t <= 60000
u >= 120%	6	3	-
120% > u >= 110%	4	-	-

Voltage Dips 3-ph:

Residual Voltage [%Vnom]	Duration [ms]				
	½cyc <= t <= 200	200 < t <= 500	500 < t <= 1000	1000 < t <= 5000	5000 < t <= 60000
90% > u >= 80%	-	3	-	-	-
80% > u >= 70%	3	-	-	-	-
70% > u >= 40%	-	-	-	-	-
40% > u >= 5%	-	-	-	-	-
5% > u >= 0%	-	-	-	-	1

Close