Manual Supplement

Manual Title:	1523, 1524 Technical Guide	Supplement Issue:	**3**
Print Date:	March 2014	Issue Date:	11/25
Revision/Date:		Page Count:	2

This supplement contains information necessary to ensure the accuracy of the above manual.

© 2014-2025 Fluke Corporation. All rights reserved..

FLUKE®
Calibration

Change #1, 367


On page 21, Table 14:

Change: ±0.030 at 600 °C

To: ±0.030 at 100 °C

Change #2, 554

On page 27, replace Figure 16 with:

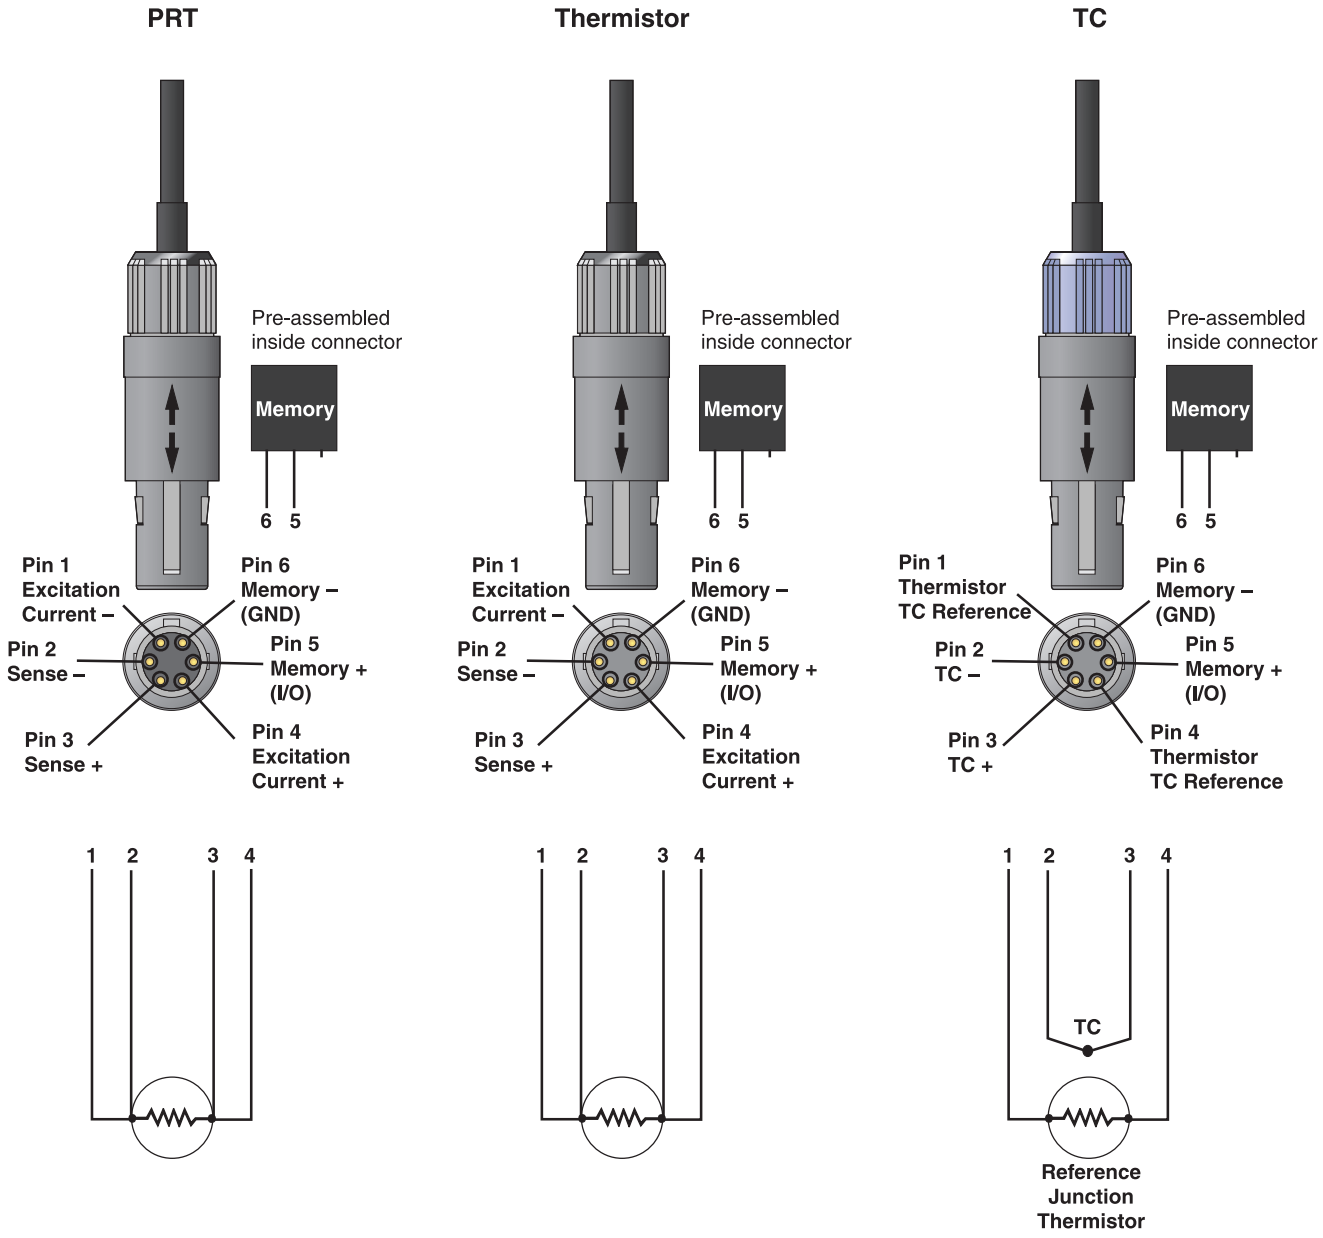

Change #3, IMCR 9-2012

On page 78, under **General**, add this before the 1st paragraph:

Be aware that multiple measurements are taken at each calibration point to provide robust statistical analysis.

On page 84, under **7.9.1.3.1 L75 Ohms Range** through page 89, **7.9.1.3.6 Reference Junction Ohms Range**, replace “Record the data” with:

Record the mean and standard deviation of the 40 measurement sample.

Change #4, Tpubs-411

On page 84, step 15, change:

CAL1:DEV:RANG:SEL MV_OHMS

To:

CAL1:DEV:RANG:SEL MV